

## CGM Device Summary


Device	Works with	Provided free through NDSS subsidy	Product lifespan	Other features
Dexcom G4 Platinum	Animas Vibe insulin pump OR Dexcom G4 Platinum Receiver	Dexcom G4/G5 Platinum Sensor	Sensor – 7 days	
		Dexcom G4 Platinum Transmitter	Transmitter – 6 months	
Dexcom G5 Mobile	Compatible iOS (Apple) or Android smartphone or smart device OR Dexcom G5 Mobile Receiver OR t:slim X2 Insulin Pump	Dexcom G4/G5 Platinum Sensor	Sensor – 7 days	Dexcom Share feature allows up to 5 people to follow the user's glucose data using the Dexcom Follow App on their mobile phone or smart device.
		Dexcom G5 Mobile Transmitter	Transmitter – 3 months	
Medtronic Guardian Connect	Compatible iOS (Apple) or Android smartphone or smart device	Enlite Sensor	Sensor – 6 days	SMS messages can be sent to up to 5 people to notify them of alerts and alarms on the user's CGM device.
		Medtronic Guardian Connect Transmitter	Transmitter – 12 months	
Medtronic Guardian Link	Medtronic Minimed 640G insulin pump	Enlite Sensor	Sensor – 6 days	SmartGuard feature can predict when glucose levels are approaching a low level and automatically stop insulin delivery from the user's pump, resuming delivery when their glucose level recovers.
		Medtronic Guardian Link Transmitter	Transmitter - 12 months	
Medtronic Minilink	Medtronic Paradigm Veo or Paradigm Real-Time insulin pumps	Enlite Sensor	Sensor – 6 days	Low Glucose Suspend feature will suspend insulin delivery from the pump if the user doesn't respond to low glucose alerts.
		Medtronic Minilink Transmitter	Transmitter - 12 months	



# Compatibility Flowchart



**How do you want to connect to your CGM device?**

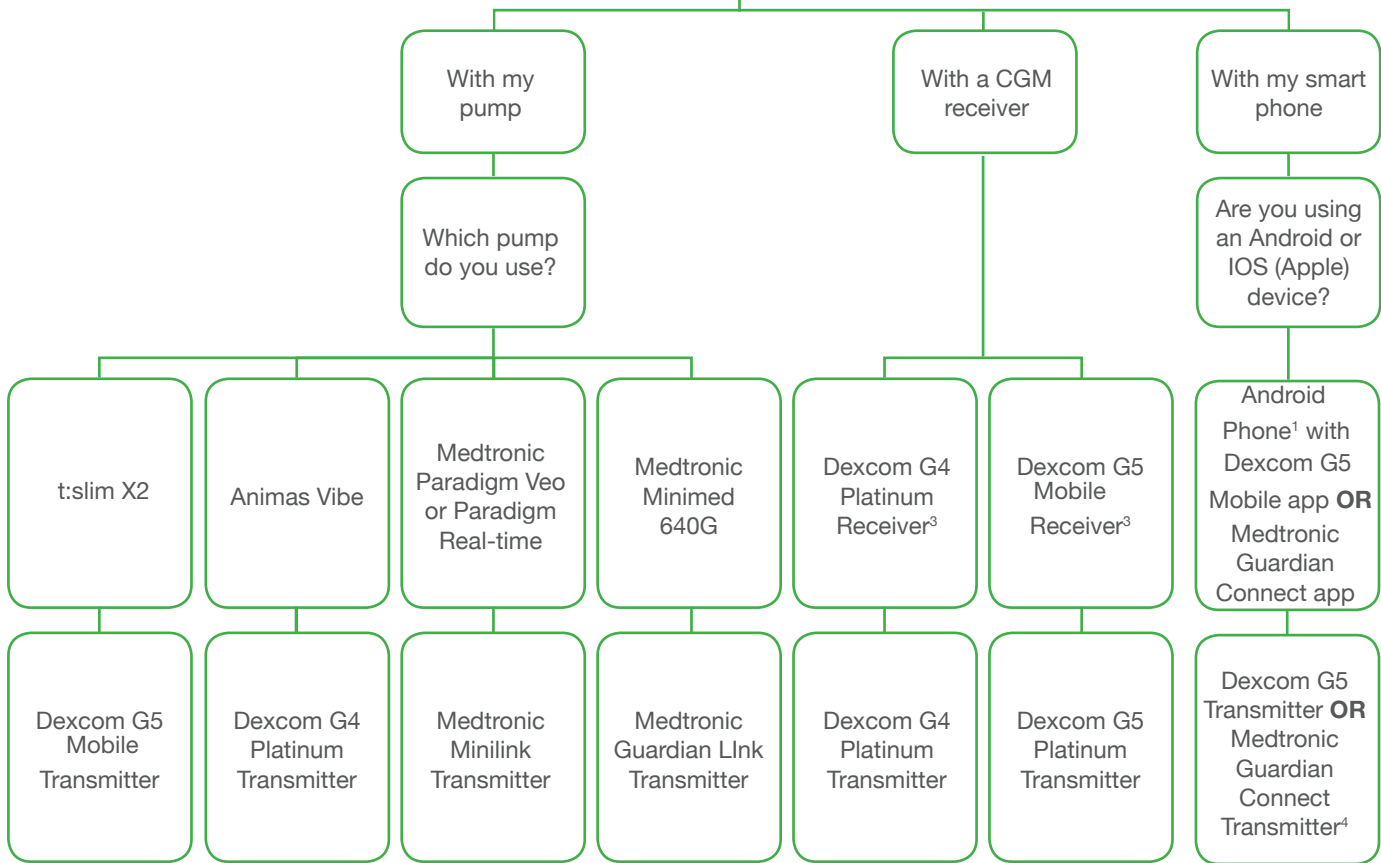

1 For information about compatible Apple iOS and Android devices for use with the Dexcom G5 Mobile visit: [dexcom.com/ous-compatibility-page](https://dexcom.com/ous-compatibility-page)  
 2 For information about compatible Apple iOS devices for use with the Guardian Connect visit: [medtronic-diabetes.com.au/guardian-connect](https://medtronic-diabetes.com.au/guardian-connect)  
 3 The Dexcom G4 Platinum and Dexcom G5 Mobile receivers are an alternative to using a compatible iOS or Android device and do not require cellular data or Wi-Fi connectivity. They are not subsidised through the NDSS Initiative and can be purchased separately through AMSL. For more details, visit [amsldiabetes.com.au/shop](https://amsldiabetes.com.au/shop).  
 4 The Medtronic Guardian Connect and Dexcom G5 Mobile transmitters must be synced to a compatible Apple iOS or Android device with Bluetooth connectivity. After syncing the apps will function without cellular data or Wi-Fi connectivity. However, for sharing services to work you will need access to regular cellular data or Wi-Fi connectivity.

# CGM Device Information and Australian Register of Therapeutic Goods (ARTG) Certificates

Device	ARTG Information	Product Information
<b>AMSL</b>		
Dexcom G4 PLATINUM	<a href="#">ARTG Certificate 169241</a>	<a href="#">Dexcom G4 Platinum User Guide</a>
Dexcom G5 Mobile	<a href="#">ARTG Certificate 169241</a>	<a href="#">Dexcom G5 Mobile User Guide</a>
<b>Medtronic</b>		
Medtronic Enlite Sensor	<a href="#">ARTG Certificate 313740</a>	<a href="#">Medtronic Enlite Sensor User Guide</a>
Medtronic Guardian Connect Transmitter	<a href="#">ARTG Certificate 118347</a>	<a href="#">Medtronic Guardian Connect User Guide</a>
Medtronic MiniLink Transmitter	<a href="#">ARTG Certificate 138452</a>	<a href="#">Medtronic MiniLink Transmitter User Guide</a>
Medtronic Guardian 2 Link Transmitter	<a href="#">ARTG Certificate 118347</a>	<a href="#">Medtronic Guardian 2 Link Transmitter User Guide</a>

